


Lab Notebook Entry from LeCroy DSO  
DSO S/N: LCRY0614N49164  
User: LeCroyUser  
Time: 12/10/2014 3:53:31 PM

12/10/2014 3:53:31 PM

TxCikOut

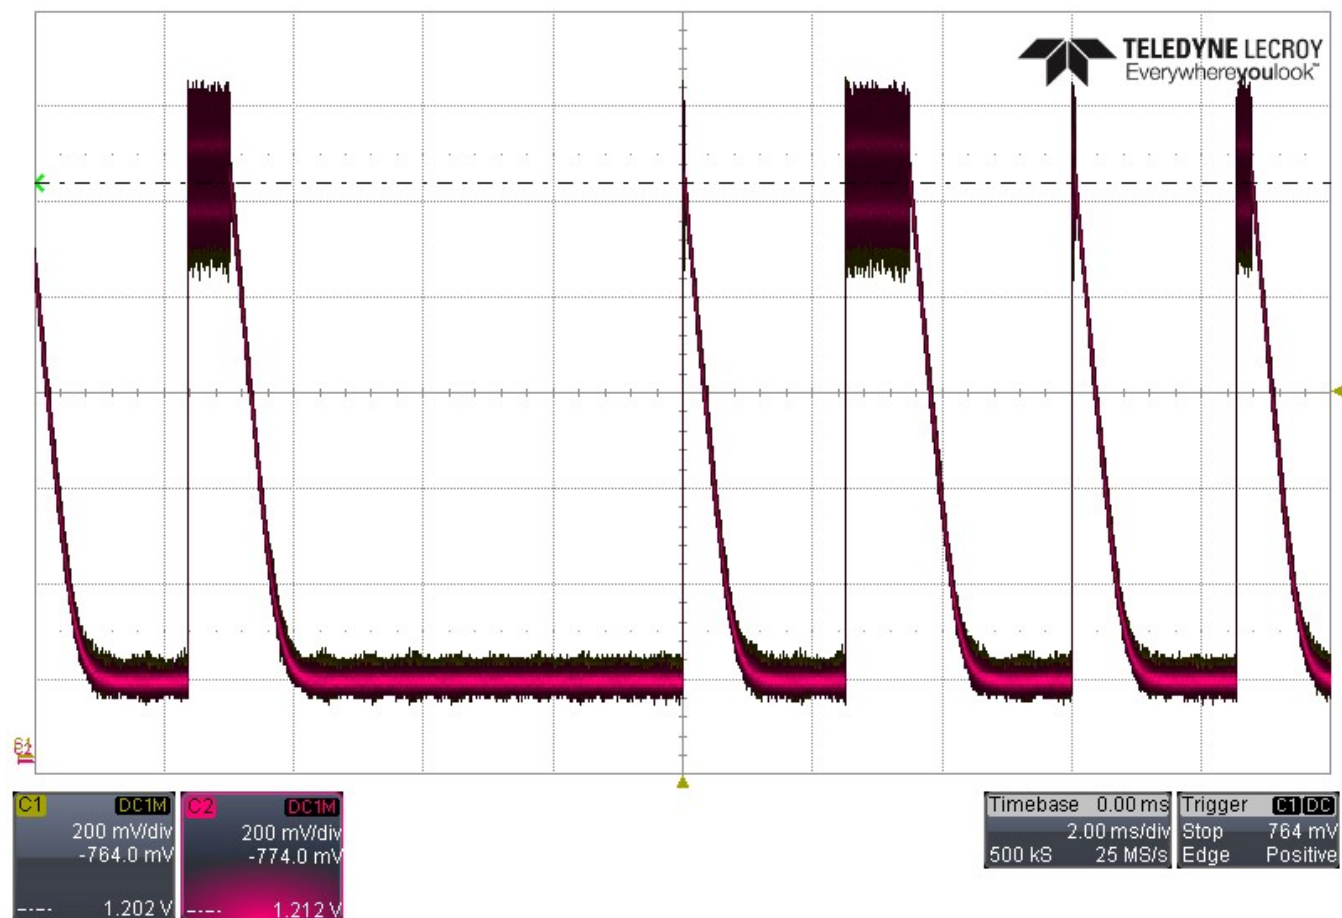

#### Channel Status

	C1	C2
Vertical	V / Div	200 mV
	Offset	-764.0 mV
	Coupling	DC1MΩ
	BW-Limit	Full
	Probe	10
	Sweeps	1 #

#### Acquisition Status

Horizontal	Time / Div	2.00 ms	Sampling Rate	25 MS/s
	Time / Pt	40.000 ns	Sampling Mode	RealTime
	Pts / Div	50.0000 kS	Trigger Delay	0.00 ms
Trigger	Mode	Stop	Slope	Positive
	Type	Edge	Level	764 mV
	Source	C1	Coupling	DC

